SOBER CHECK LTD

Specialists in drug & alcohol testing solutions

CT Oral Scan Procedure

STEP 1

Using the provided collection swab, remove the collector from the sealed pouch, have donor sweep inside of mouth (cheek, gum, tongue) several times, then hold swab in mouth until colour on the saturation indicator strip appears in the indicator window of collection swab. **Important: Do not bite, suck, or chew on the sponge.**

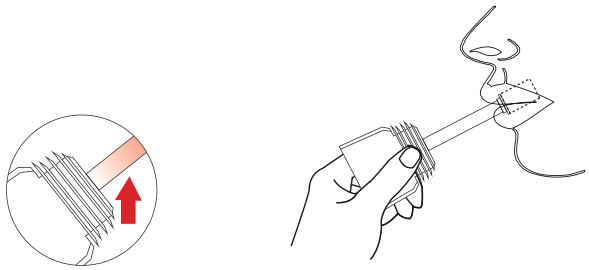

Note: If after 5 minutes, colour on the saturation indicator has not appeared in the indicator window, proceed with step 2 of the test.

STEP 2

Place the test device on a clean and flat surface. Remove the collection sponge from the mouth and insert the sponge first into the screening device **gently and slowly,** press until the collector cap sealed with the device tightly. **Keep upright when inserting the sponge.**

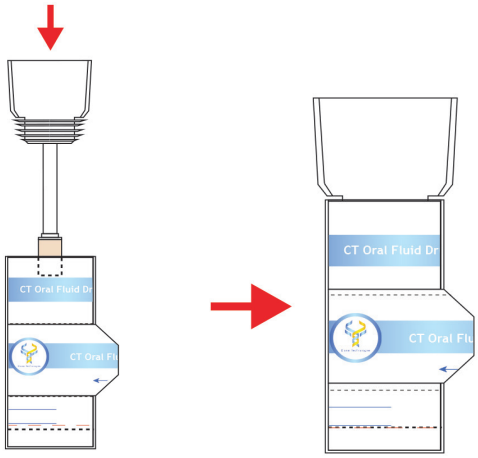

STEP 3

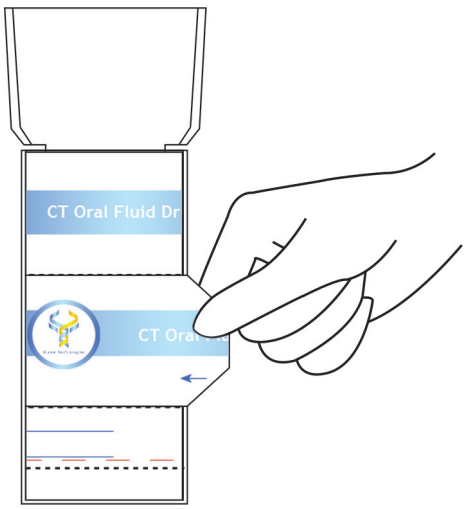

STEP 4
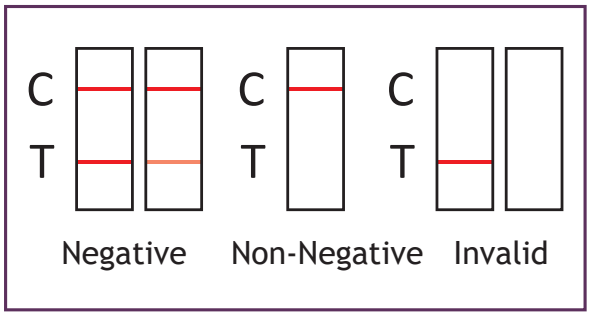
Read the results at 3 - 5 minutes.